

FIG. 1A

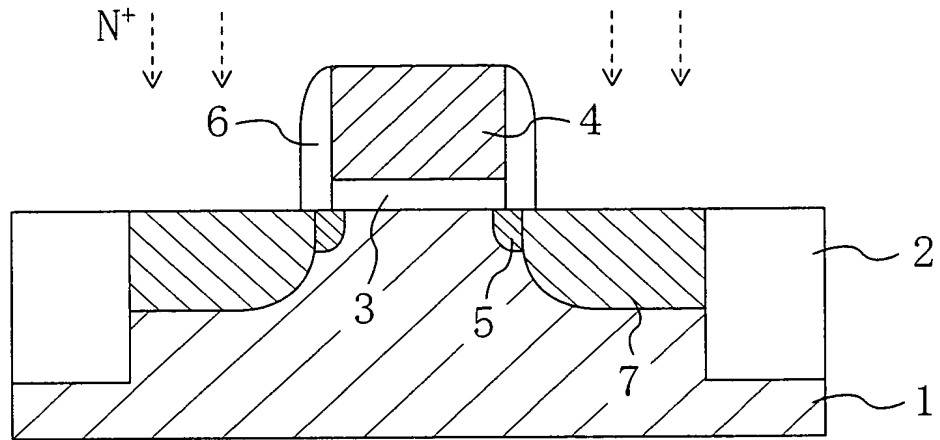


FIG. 1B


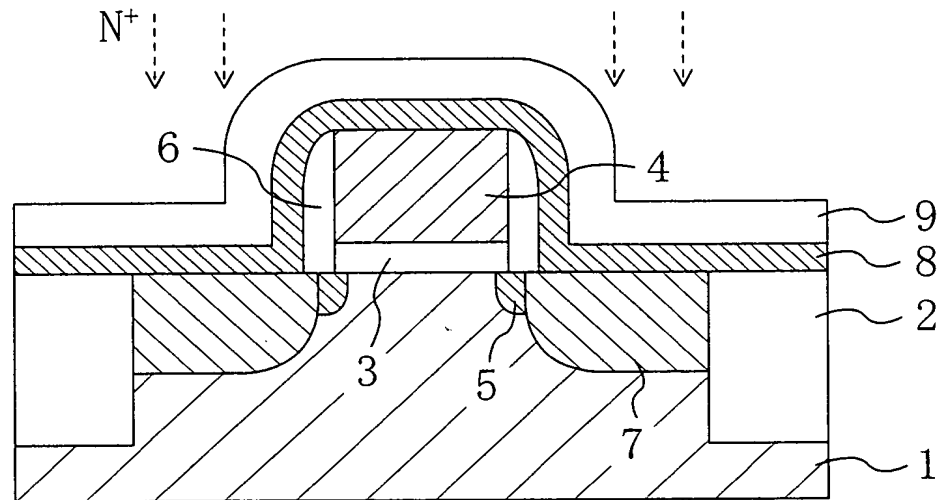


FIG. 1C

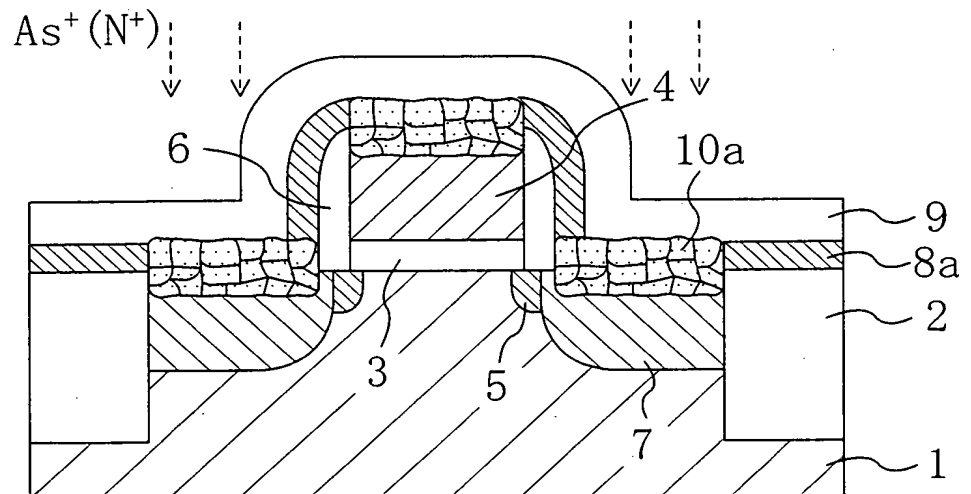

0966744-100101

APPROVED	C.G. FIG.	
BY	CLASS	SUBCLASS
DRAFTSMAN		

FIG. 2A

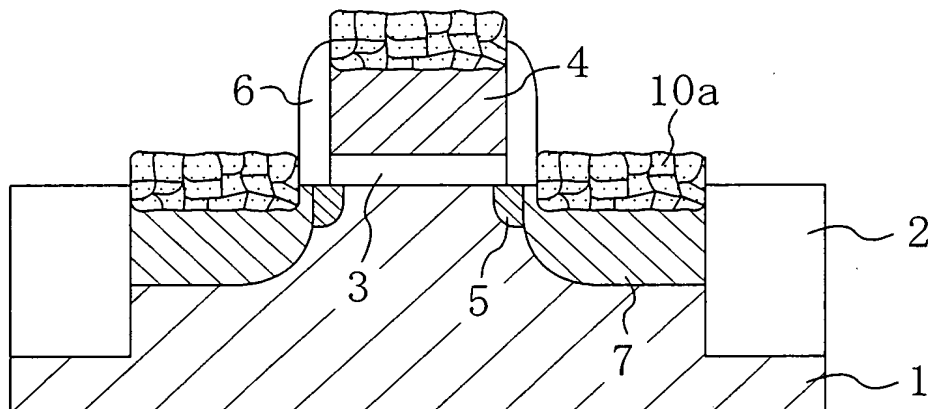


FIG. 2B


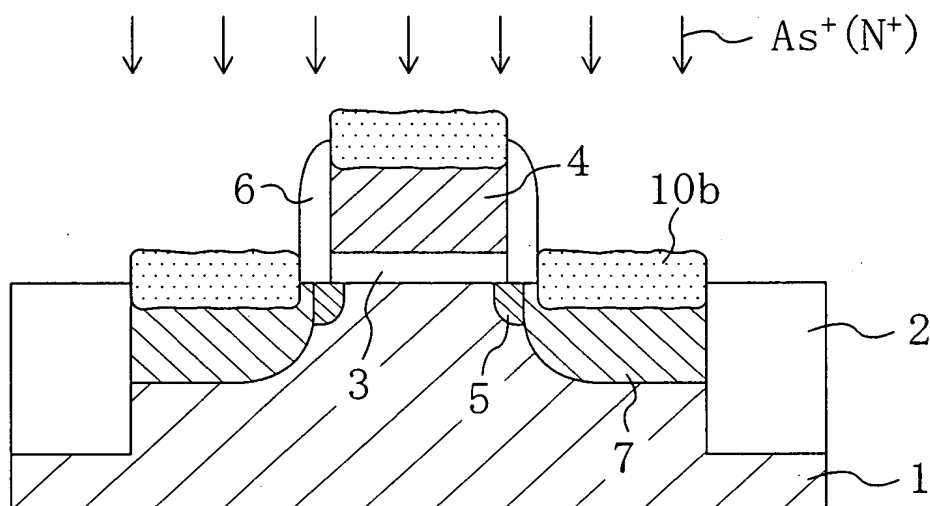


FIG. 2C

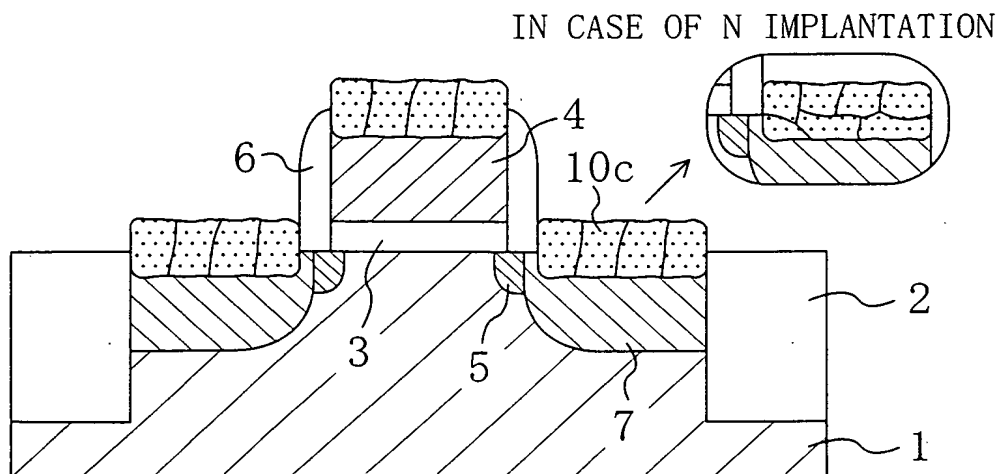

0966741-100101

FIG. 3A

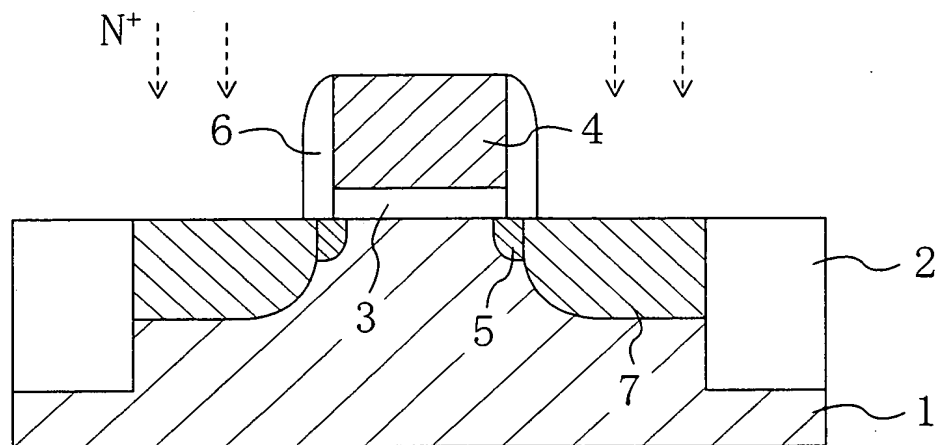


FIG. 3B


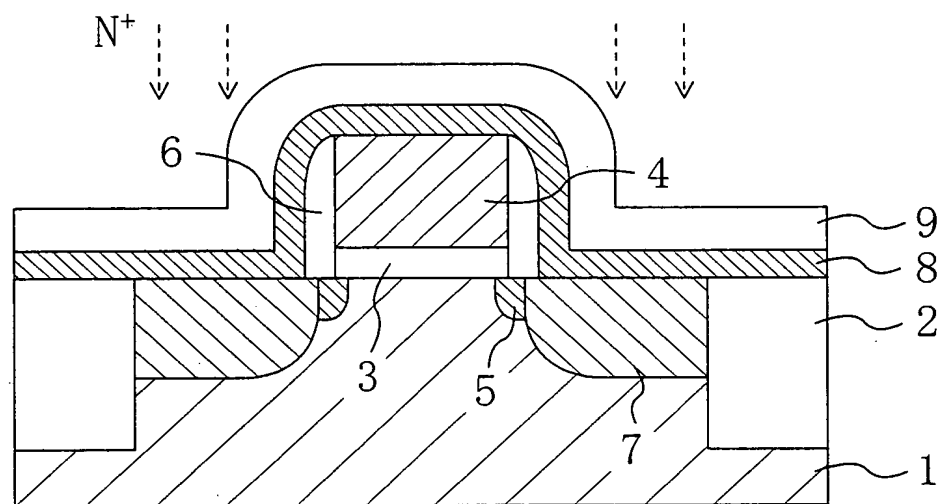


FIG. 3C

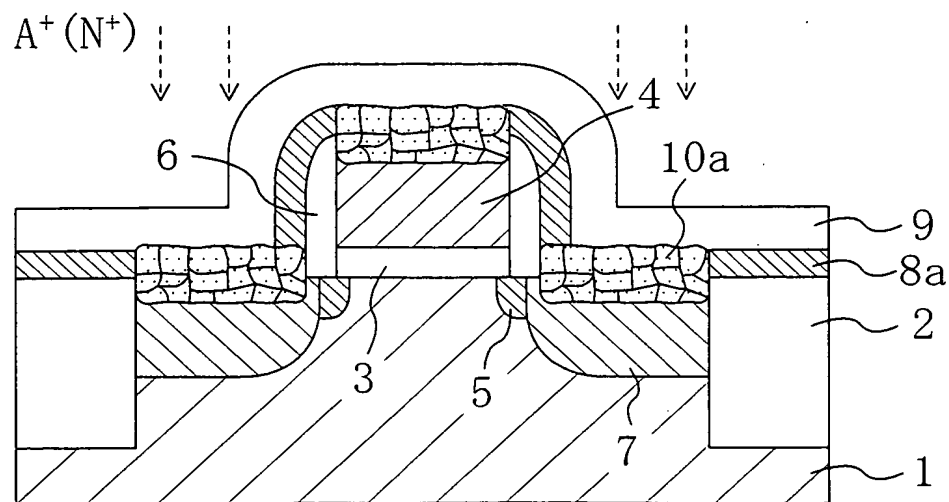

0966744-100101

FIG. 4A

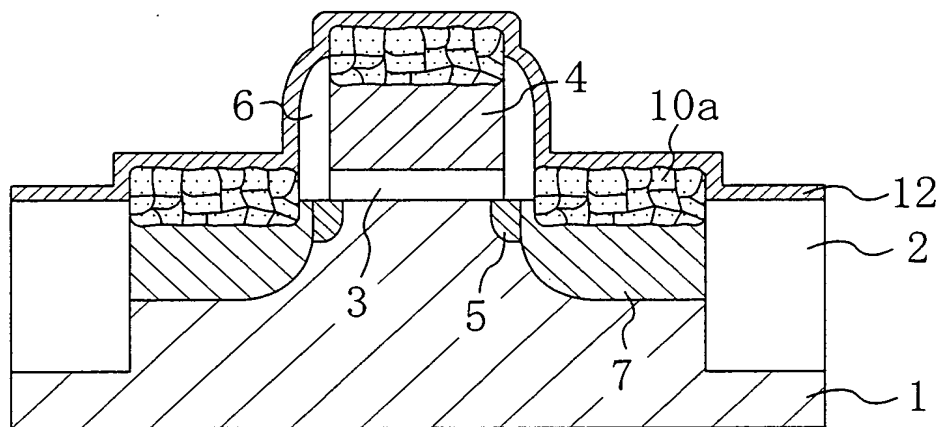


FIG. 4B


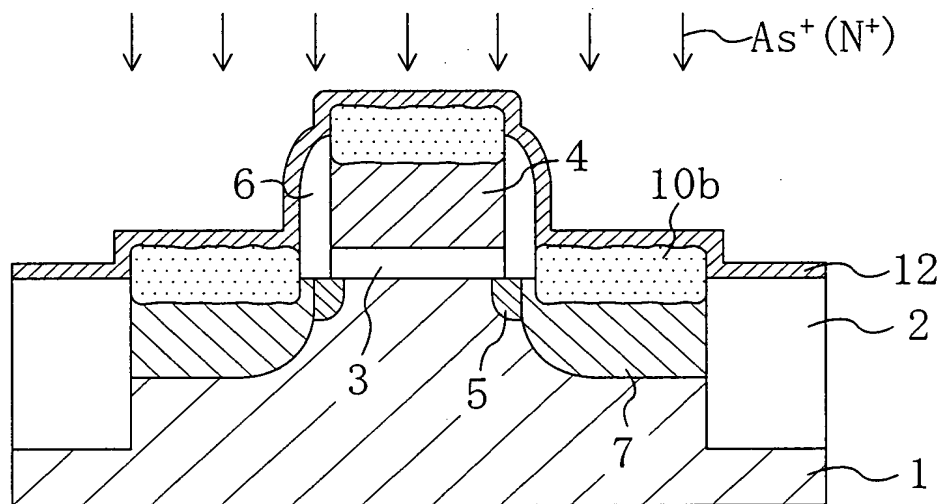


FIG. 4C

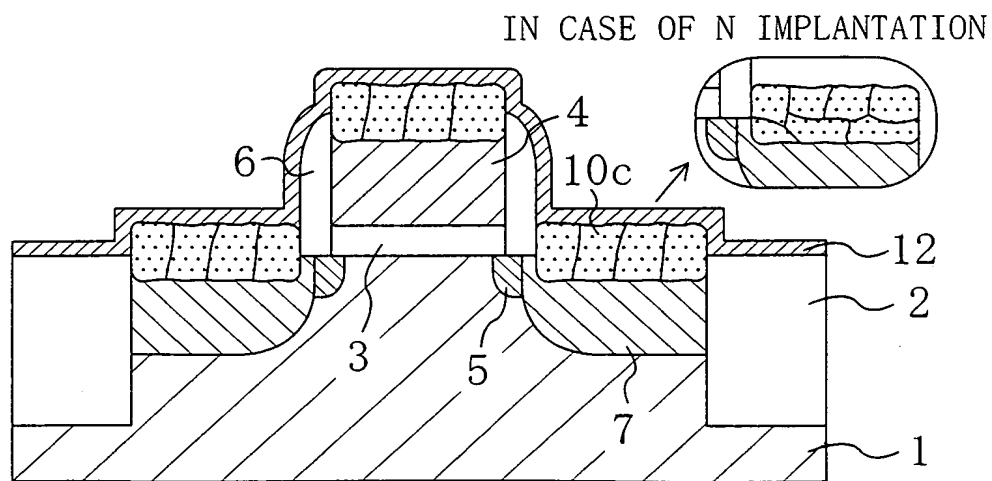

0996741-100101

FIG. 5A

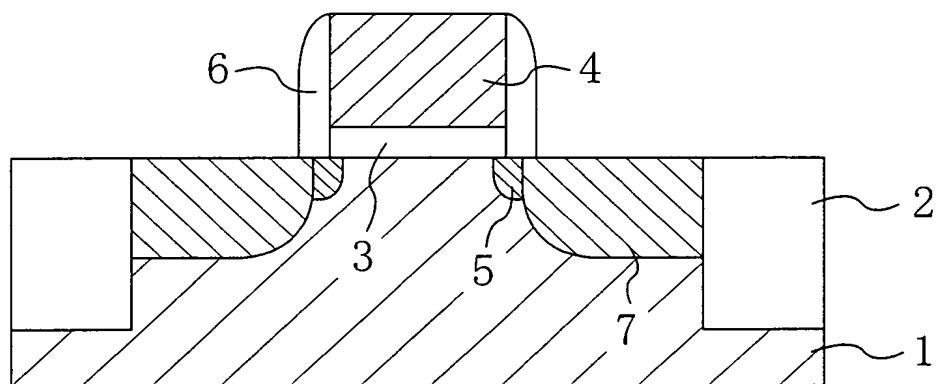


FIG. 5B


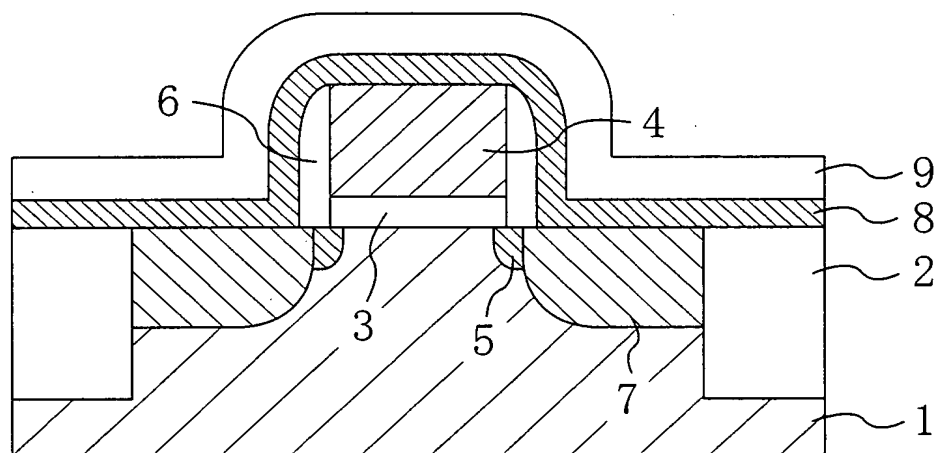


FIG. 5C

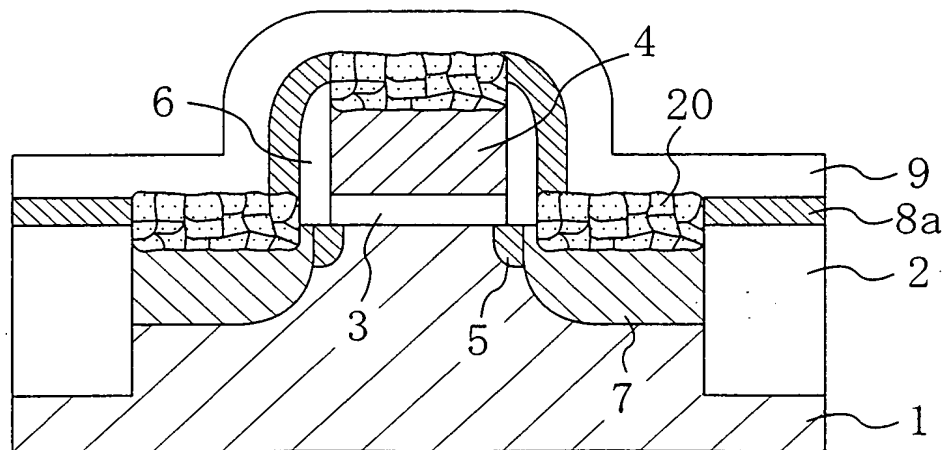

096544-100101

FIG. 7A

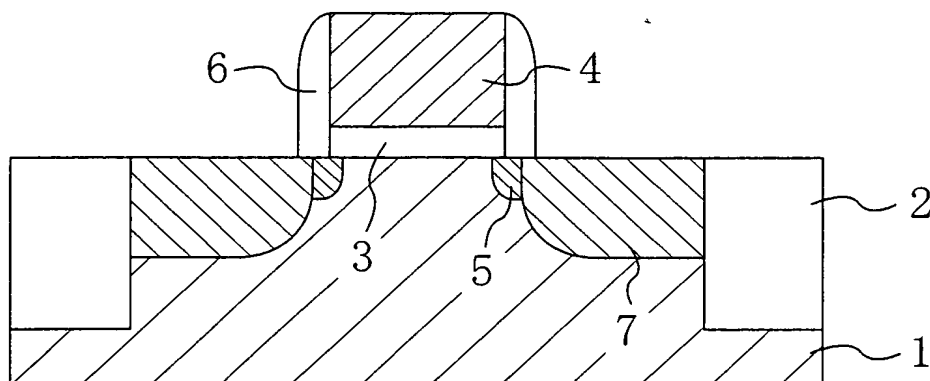


FIG. 7B

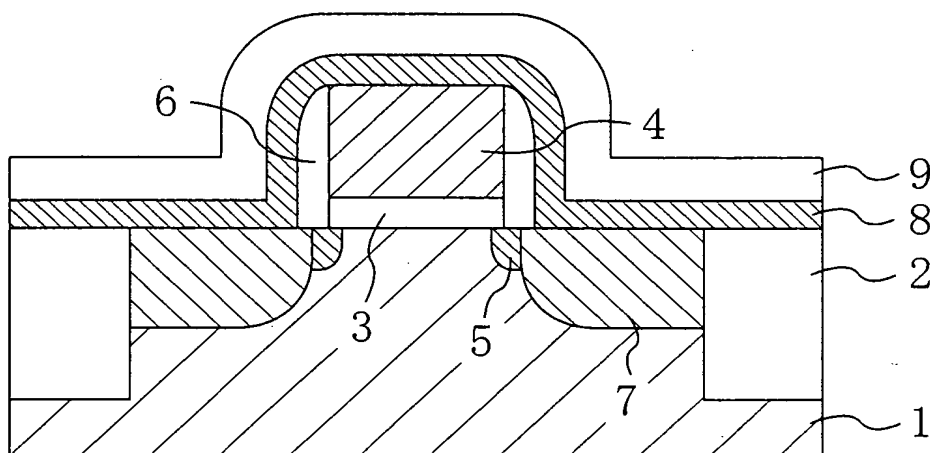


FIG. 7C

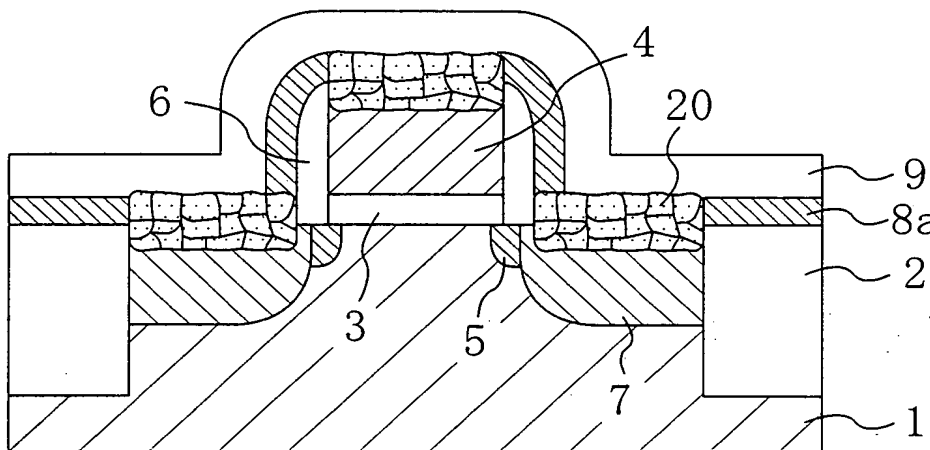


FIG. 7A

FIG. 8A

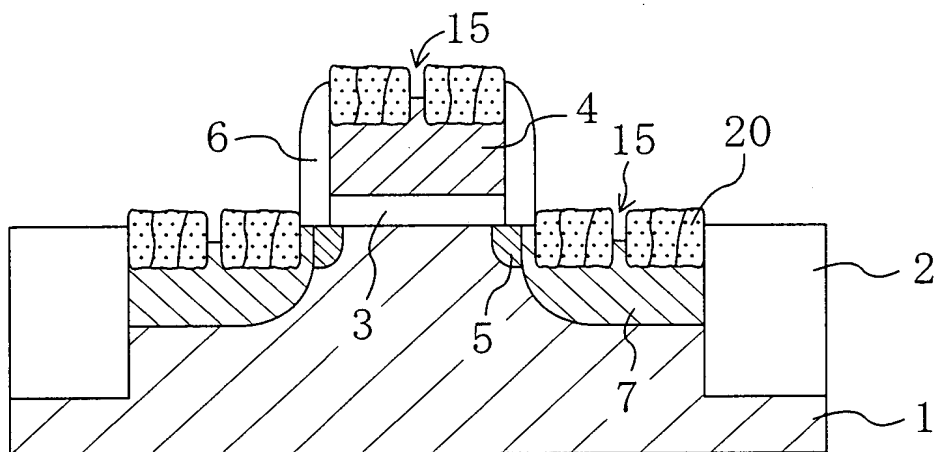


FIG. 8B

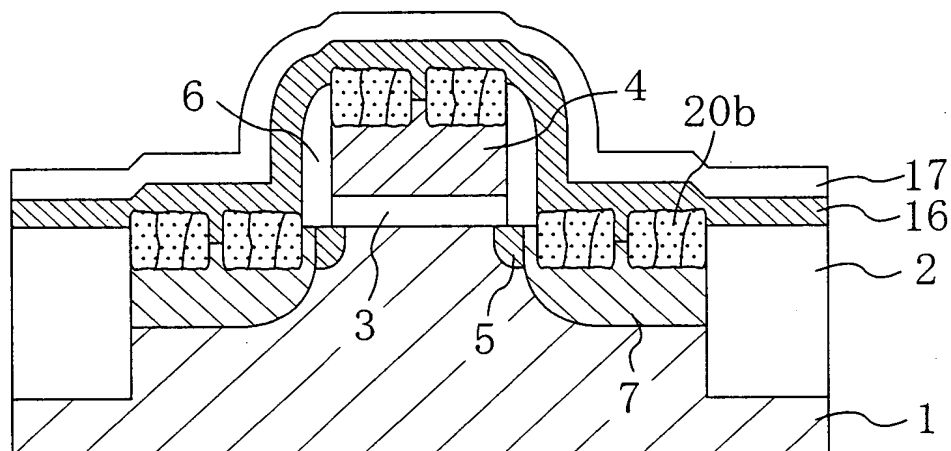


FIG. 8C

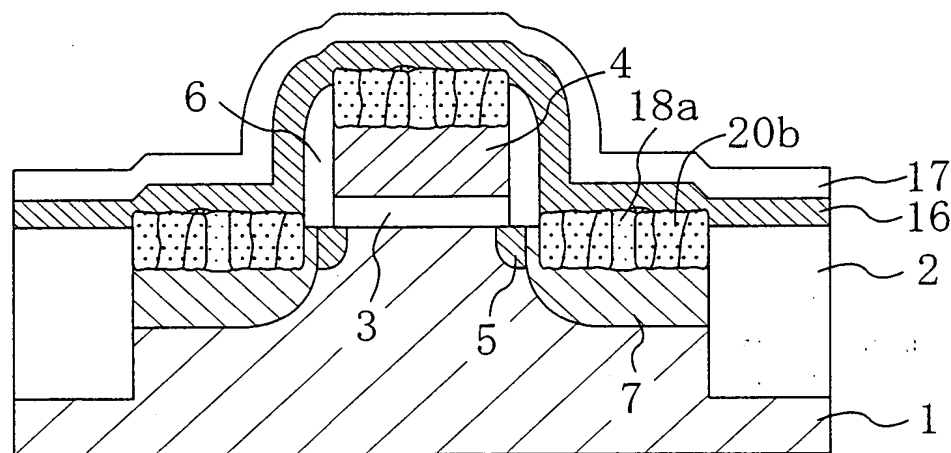


FIG. 9A

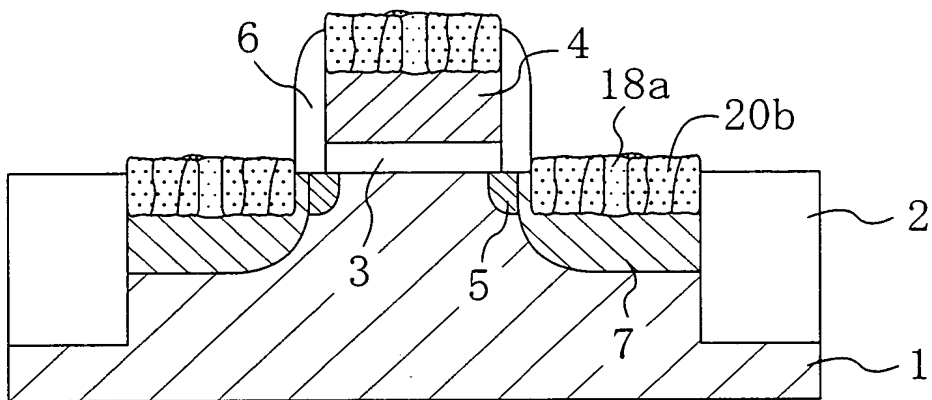


FIG. 9B

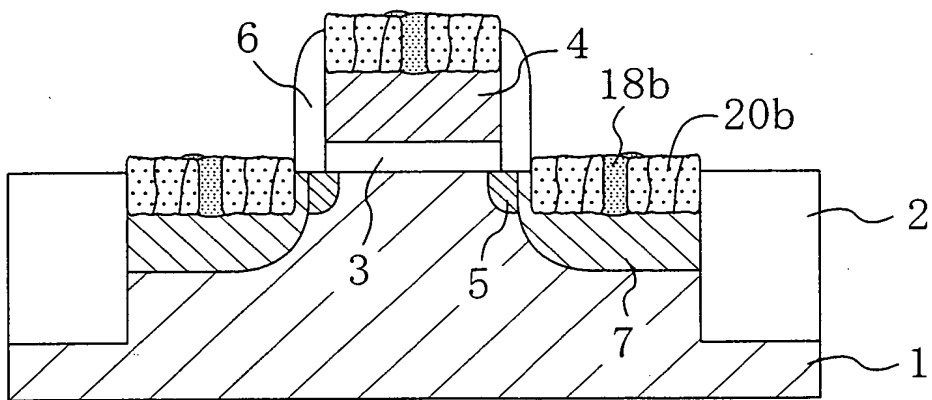


FIG. 10A
PRIOR ART

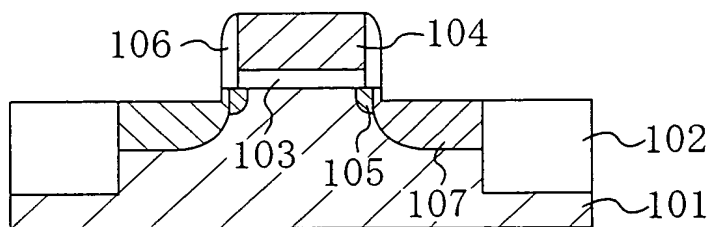


FIG. 10B
PRIOR ART

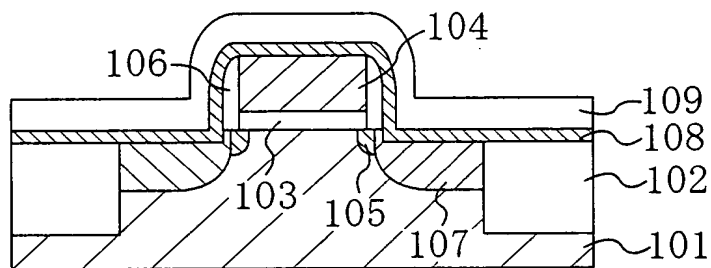


FIG. 10C
PRIOR ART

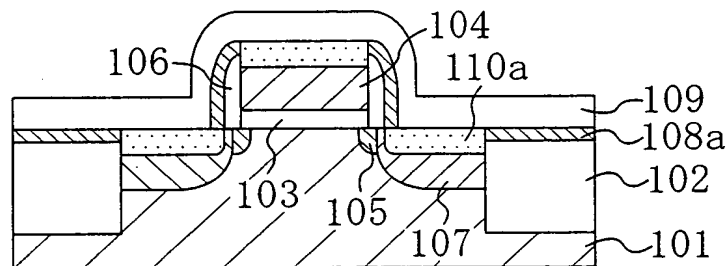


FIG. 10D
PRIOR ART

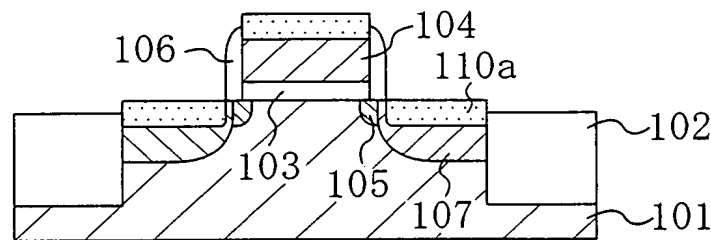


FIG. 10E
PRIOR ART

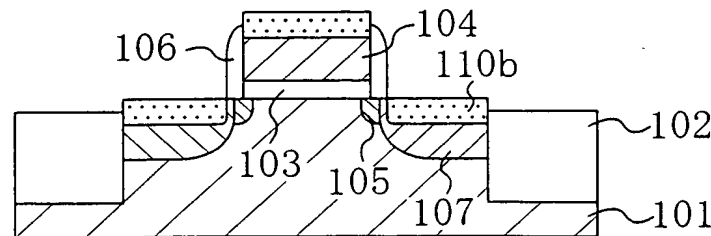


FIG. 10A

FIG. 11A
PRIOR ART

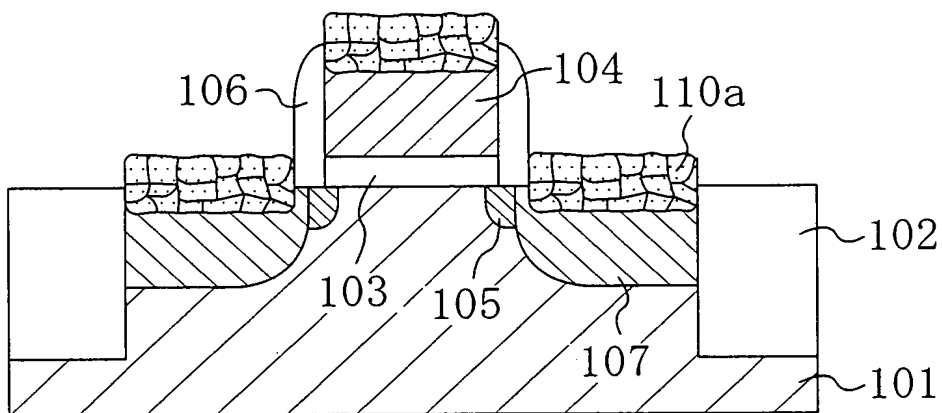


FIG. 11B
PRIOR ART

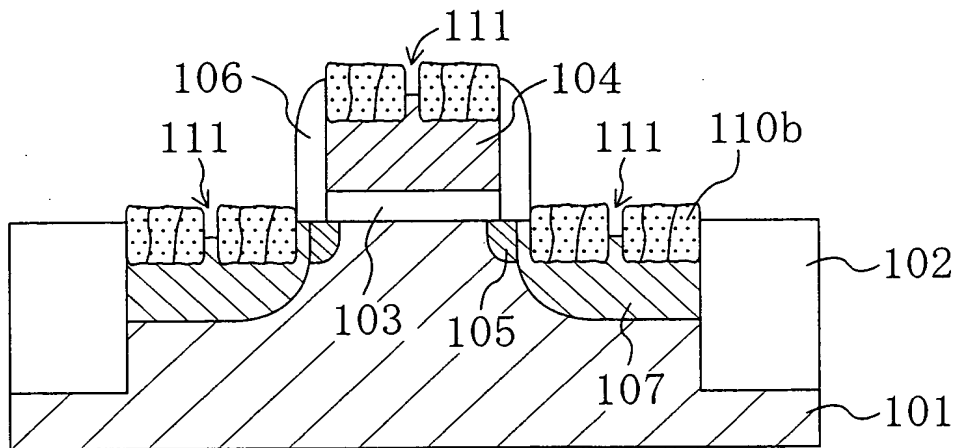


FIG. 11A

FIG. 12


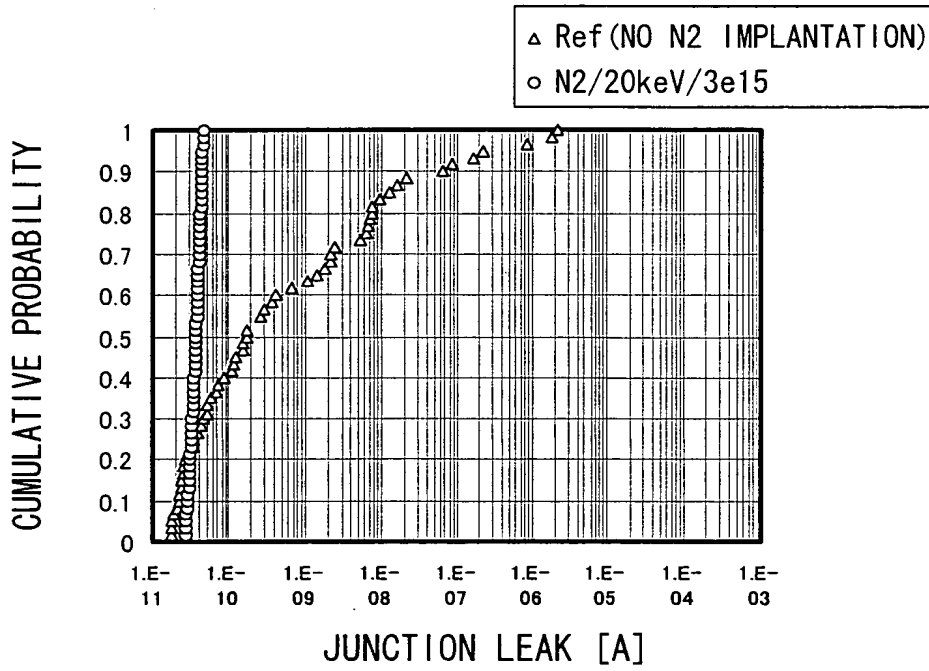


FIG. 13

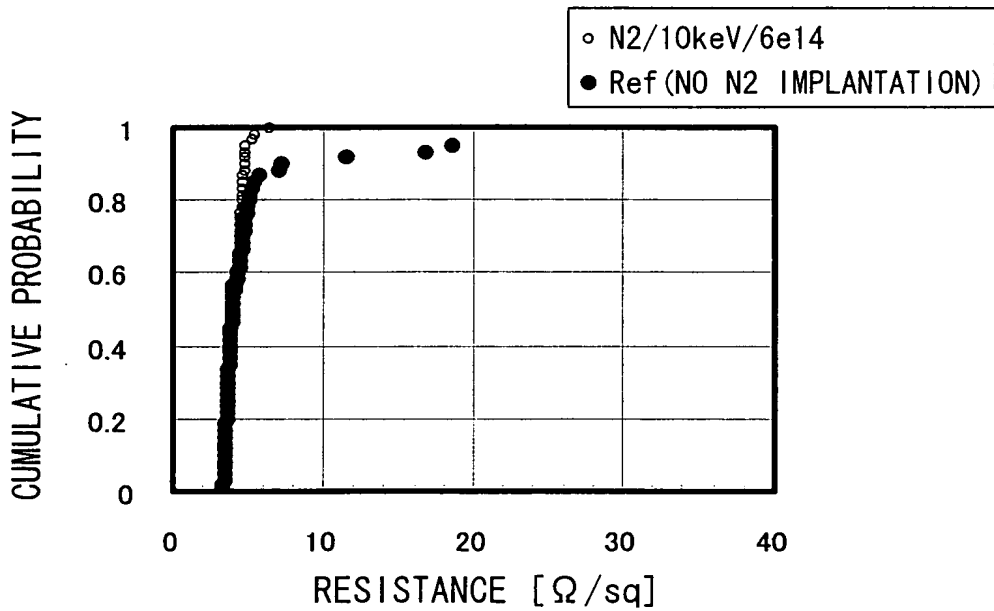

APPROVED	G. S. FRO
BY	CLASS
DR. FTSMAN	SUBCLASS

FOOT-4293660

FIG. 14A




N2 implanted CoSi2

FIG. 14B



FIG. 14C

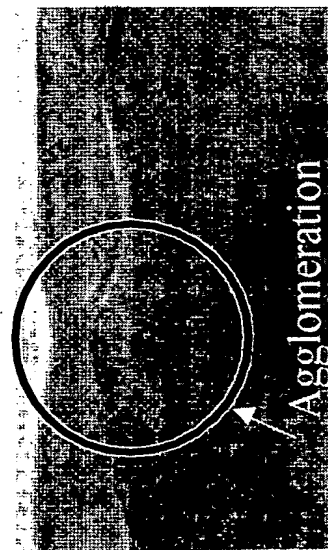

Conventional CoSi2

FIG. 14D

